

HPLC Separation Improvements for Short Chain PFAS

Conner McHale¹, Barry Boyes¹, Charles Powley²
 Advanced Materials Technology Inc., Wilmington, DE¹
 Center for PFAS Solutions, New Castle, DE²



ASMS 2024: MP- 136

Introduction

Per- and polyfluoroalkyl substances (PFAS) are a group of chemicals used to make fluoropolymer coatings and products that resist heat, oil, stains, grease, and water. These toxic “forever chemicals” are a concern to our health and environment and are now being regulated by the Environmental Protection Agency.

Short chain PFAS such as trifluoroacetic acid (TFA) are challenging to separate due to low retention and poor peak shape. Some techniques such as mixed mode hydrophilic interaction liquid chromatography (HILIC) have been demonstrated to show improved retention, however, these techniques have their limitations.


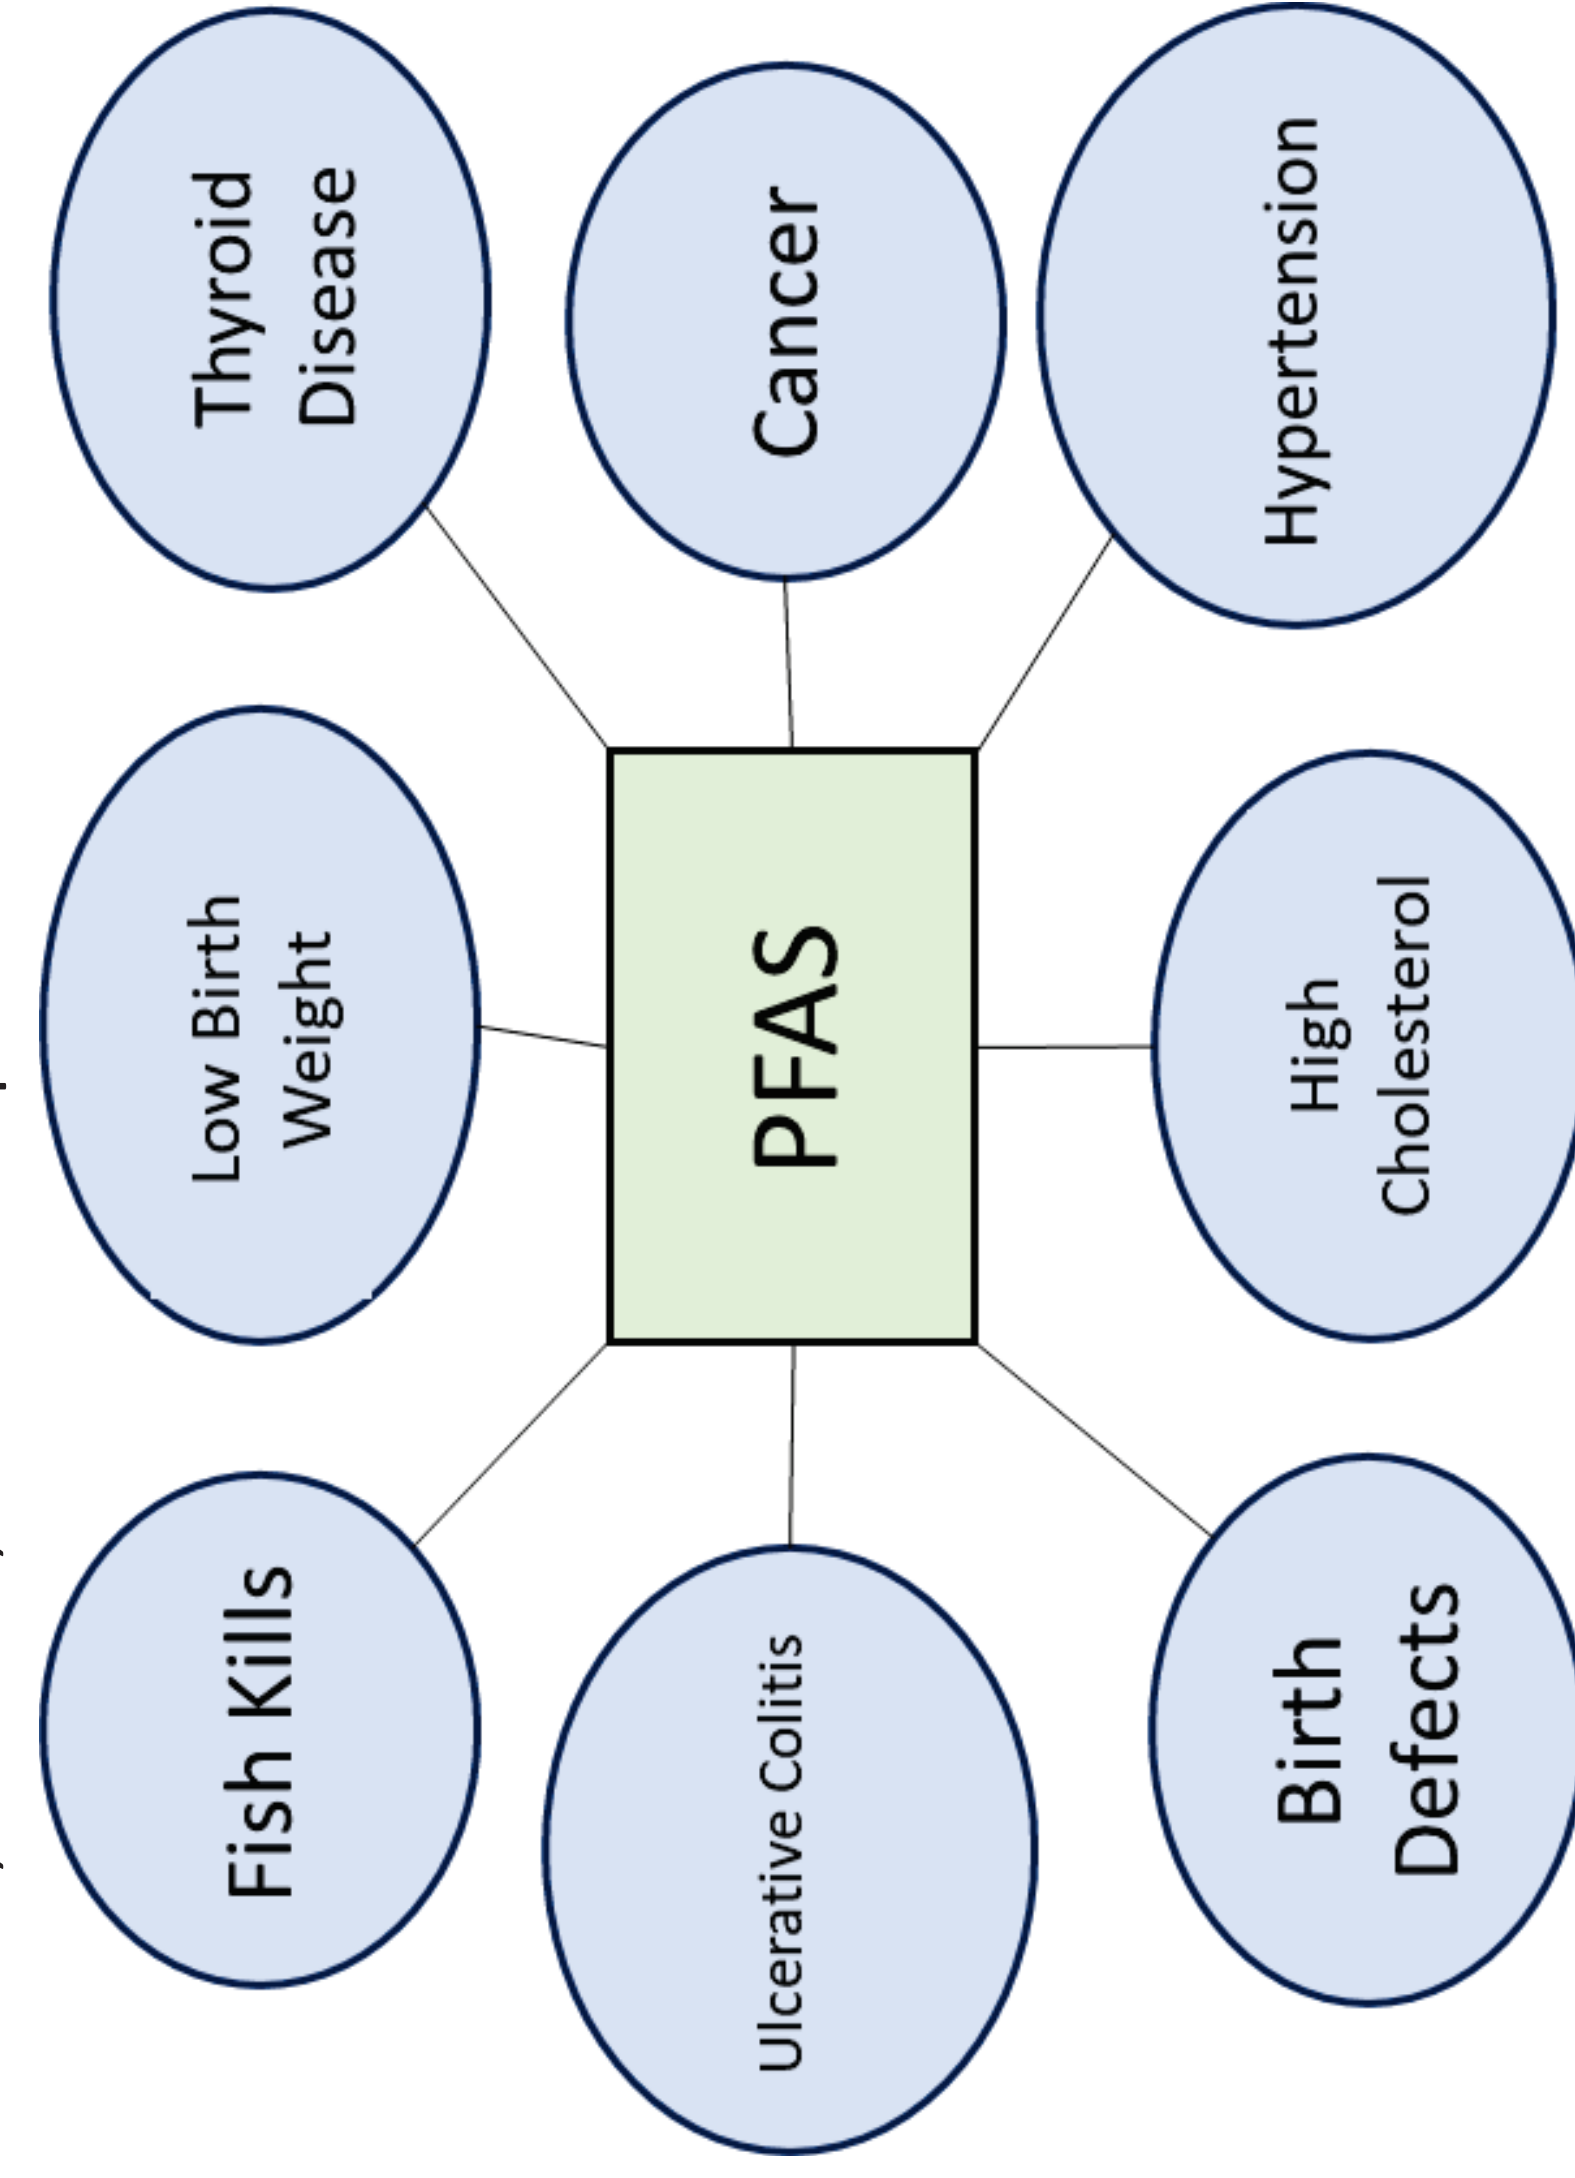



Figure 1: Common pathways for PFAS exposure released into the environment and health effects linked to PFAS

A new reverse phase, superficially porous particle (SPP) with a positive charge surface chemistry incorporated has shown separation advantages for short chain PFAS while using low ionic strength mobile phases such as formic/acetic acid.

- Excellent peak shape and increased loading capacity for basic compounds
- Alternate L1 selectivity (PCS C18)
- Alternate L1.1 selectivity (PCS Phenyl-Hexyl)
- Built upon Fused-Core® technology for fast, efficient and reliable separations


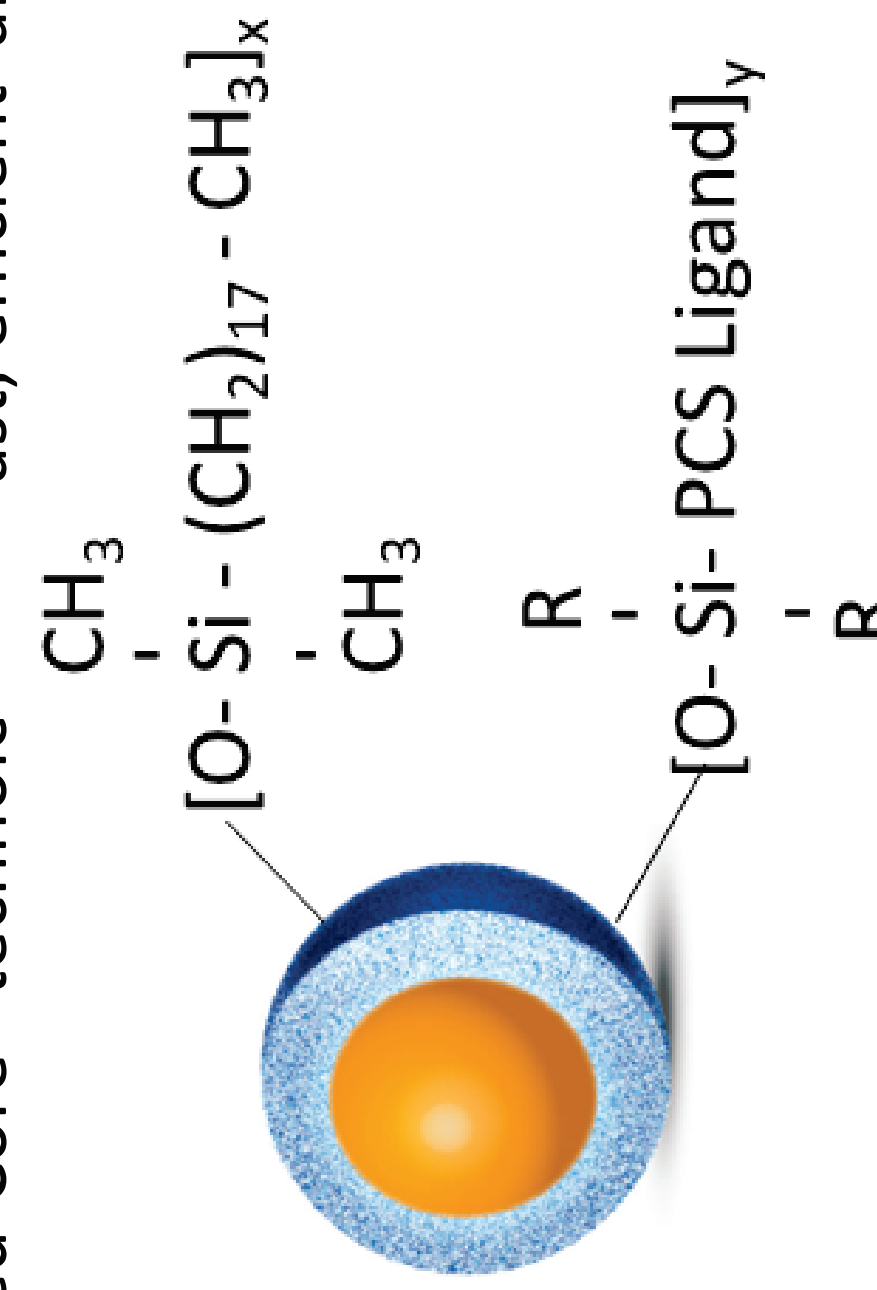


LC/MS Method Optimization

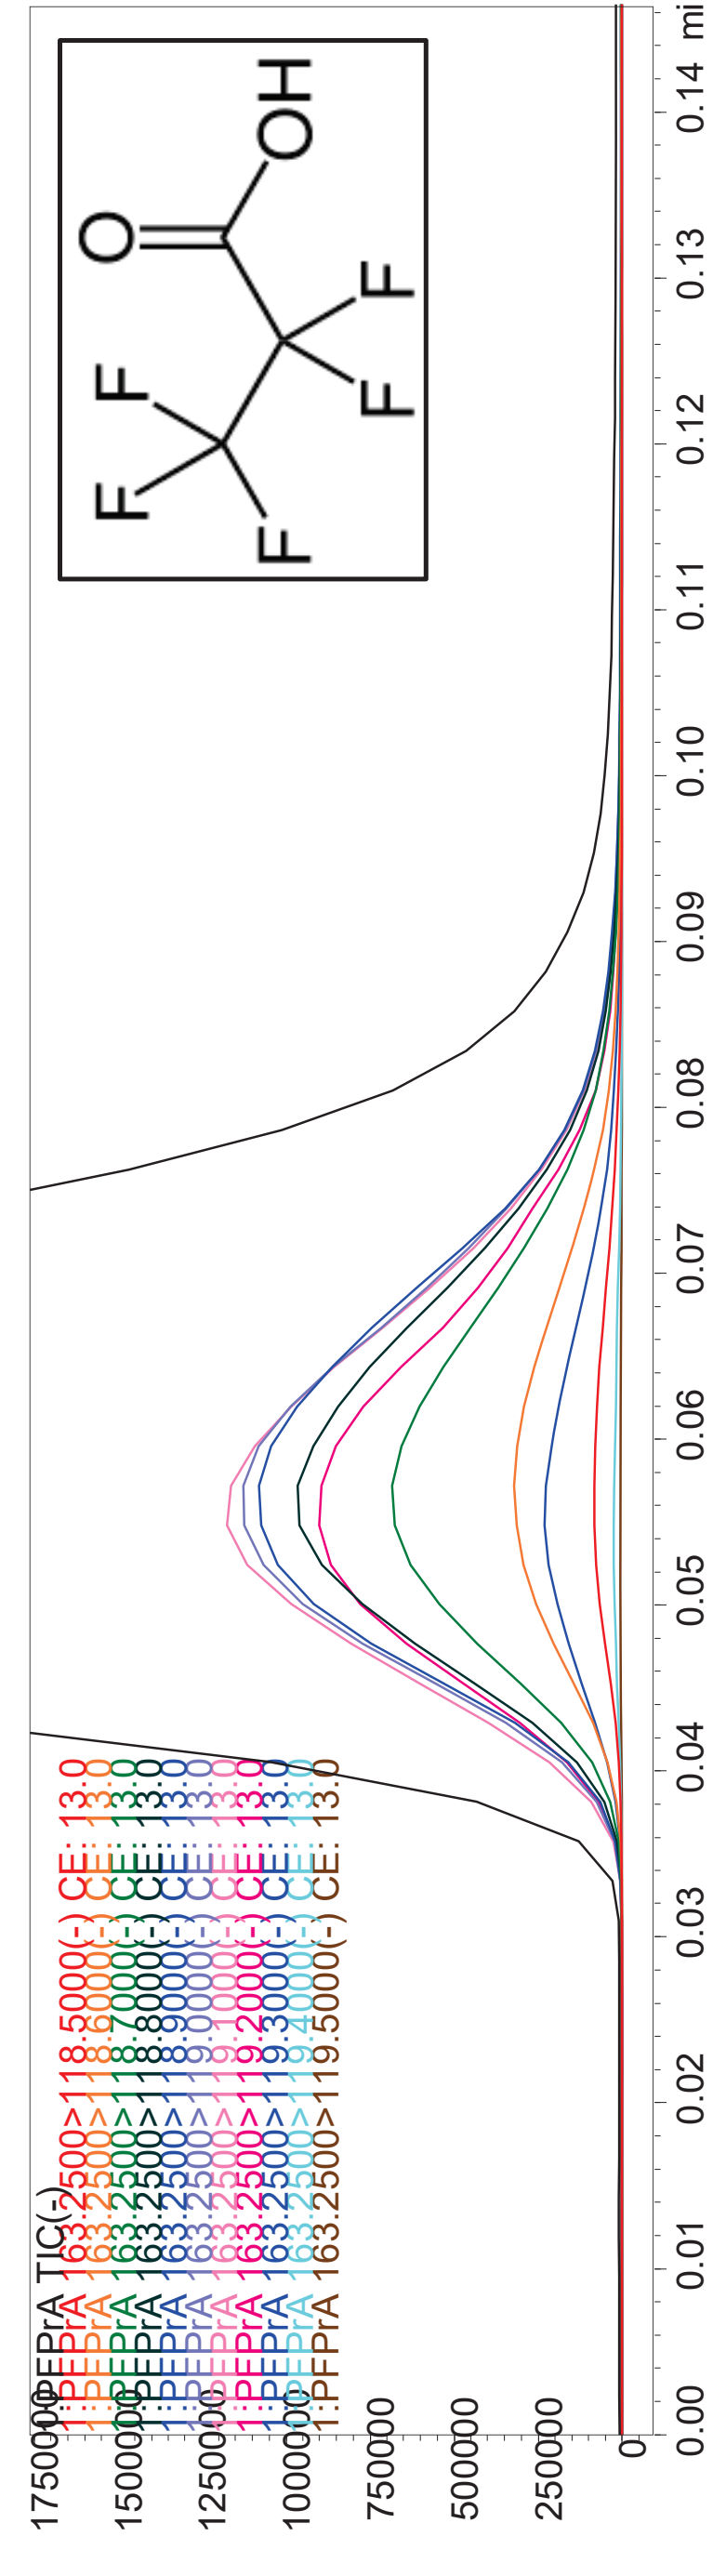


Trifluoroacetic acid (TFA) is an organofluorine compound and considered an ultra-short chain perfluoroalkyl carboxylic acid. One challenge analyzing TFA is having enough retention on column.

Perfluoropropionic acid (PFPPA) is an ultra-short chain perfluoroalkyl carboxylic acid. PFPPA is optimized on a Shimadzu 8045 LC/MS.

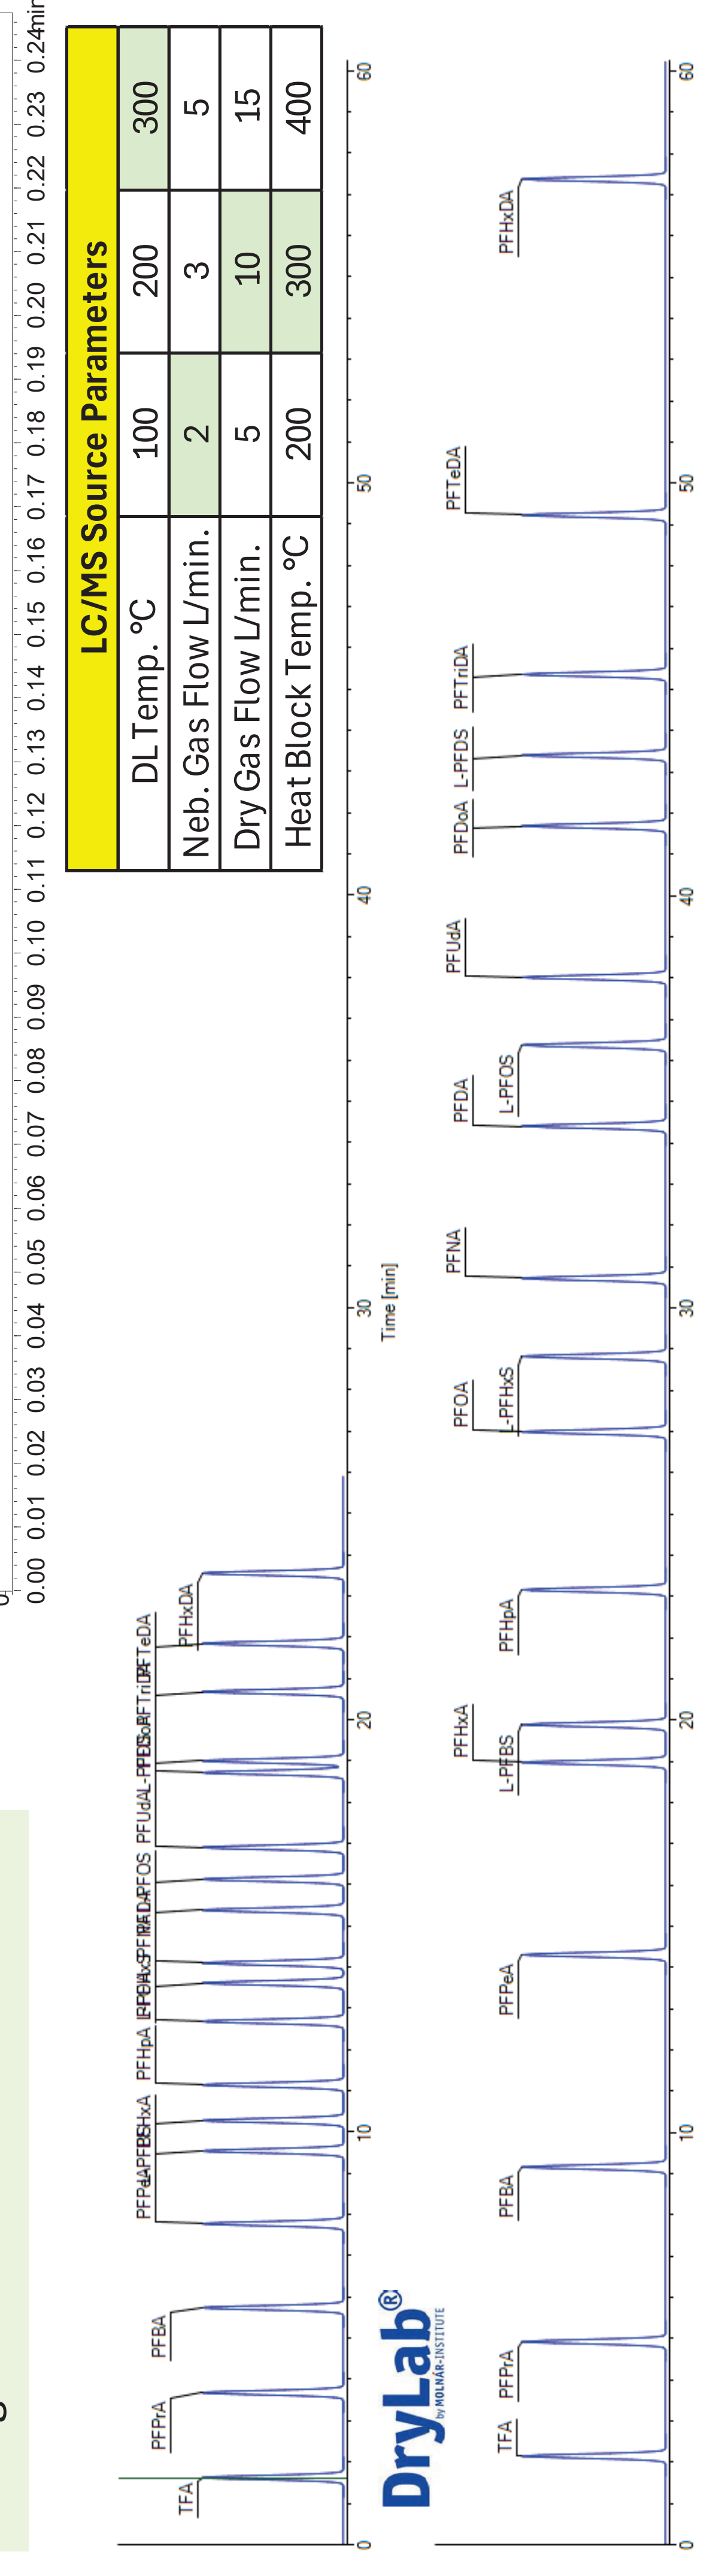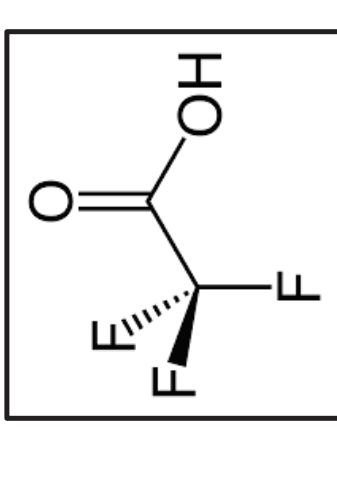


DryLab® software is utilized in order to determine adequate retention and resolution for a panel of 18 per and polyfluorinated compounds.

Superficially Porous (SPP) vs. Fully Porous Particles (FPP)

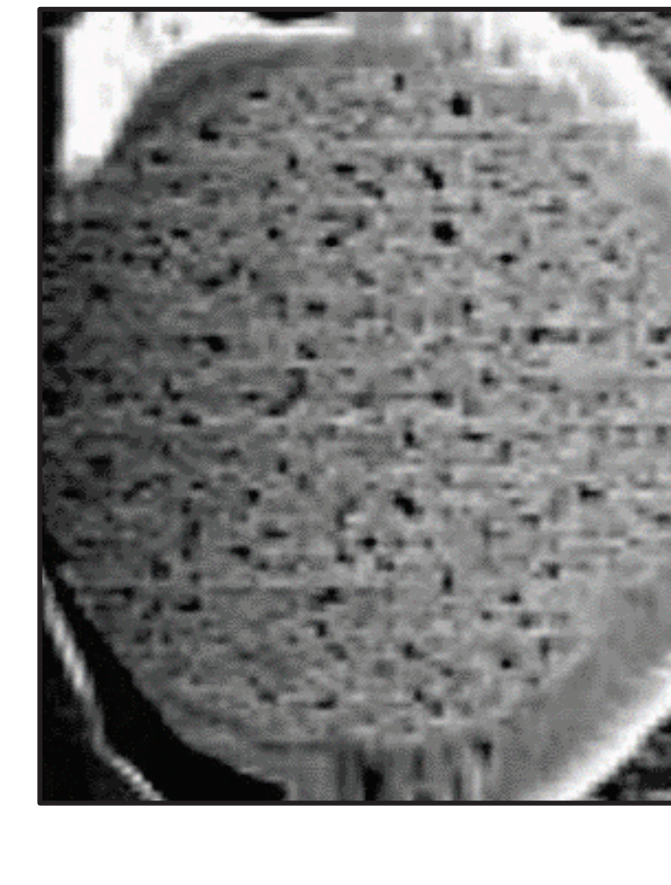


Superficially Porous Particle (SPP)

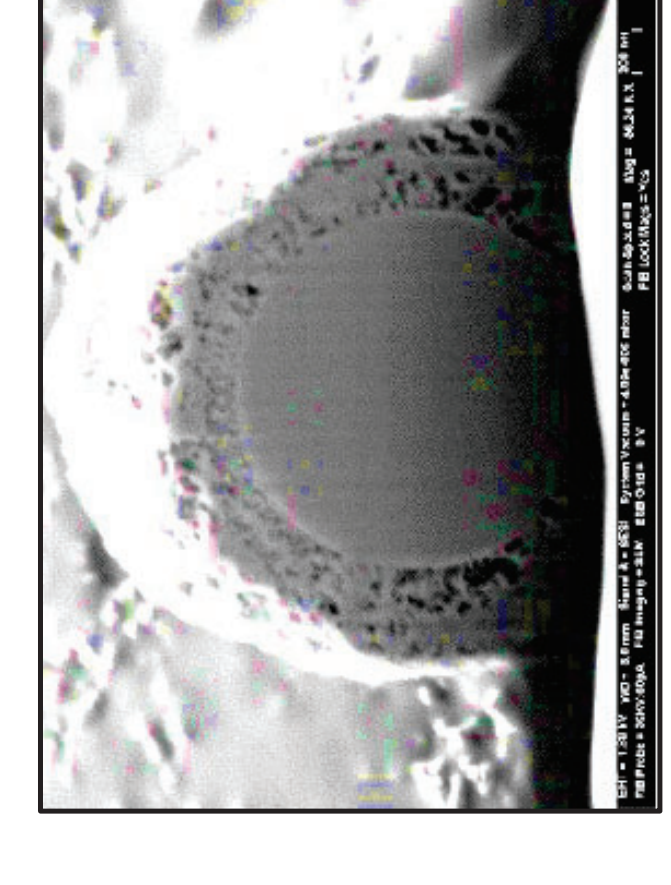

Fully Porous Particle (FPP)


Reverse Phase Positive Charge Surface: Formic Acid

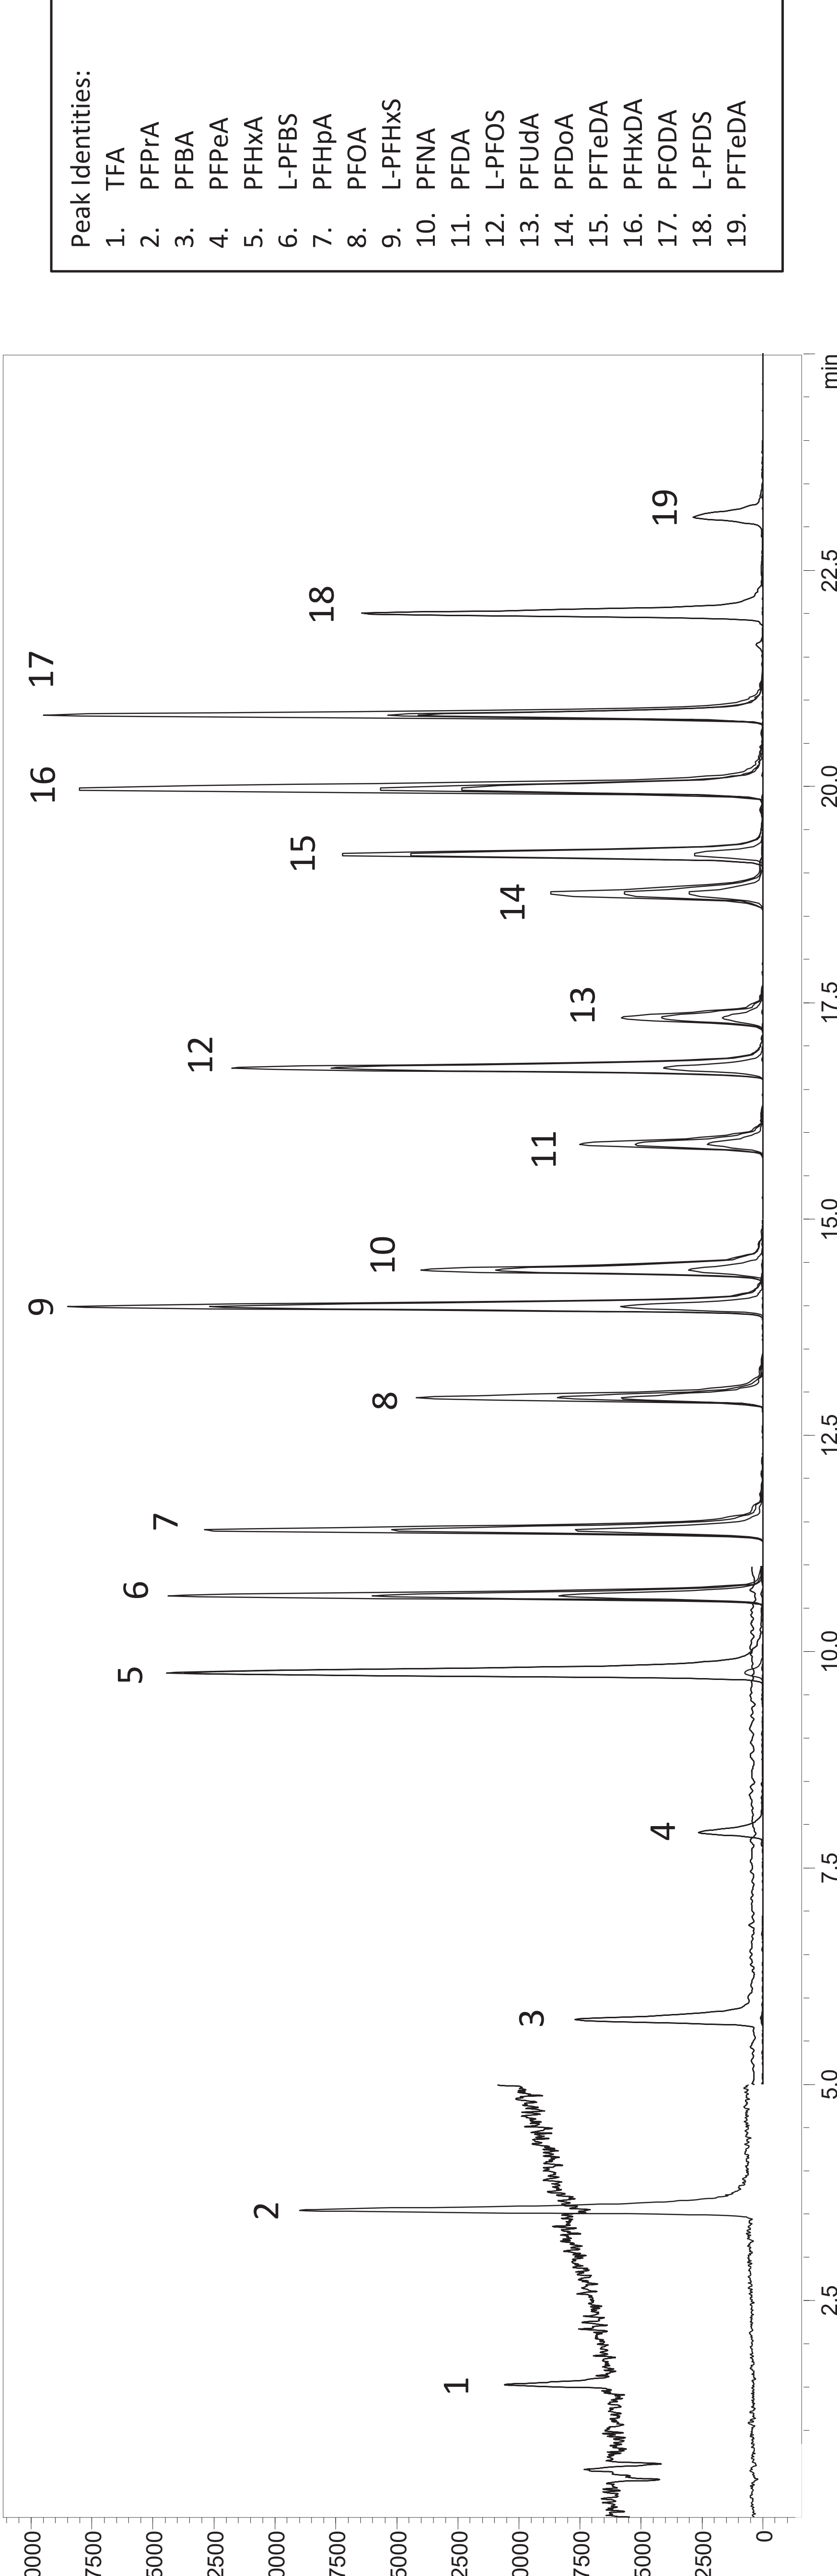

A separation of 19 per and polyfluorinated compounds including TFA and PFPPA is performed on a HALO® PCS C18 column under formic acid conditions.

Flow Rate: 0.4 mL/min
 Temperature: 35 °C
 Wavelength: PDA, 260
 LC System: Shimadzu Nexera X2
 MS System: Shimadzu 8045

Reverse Phase Positive Charge Surface: Acetic Acid

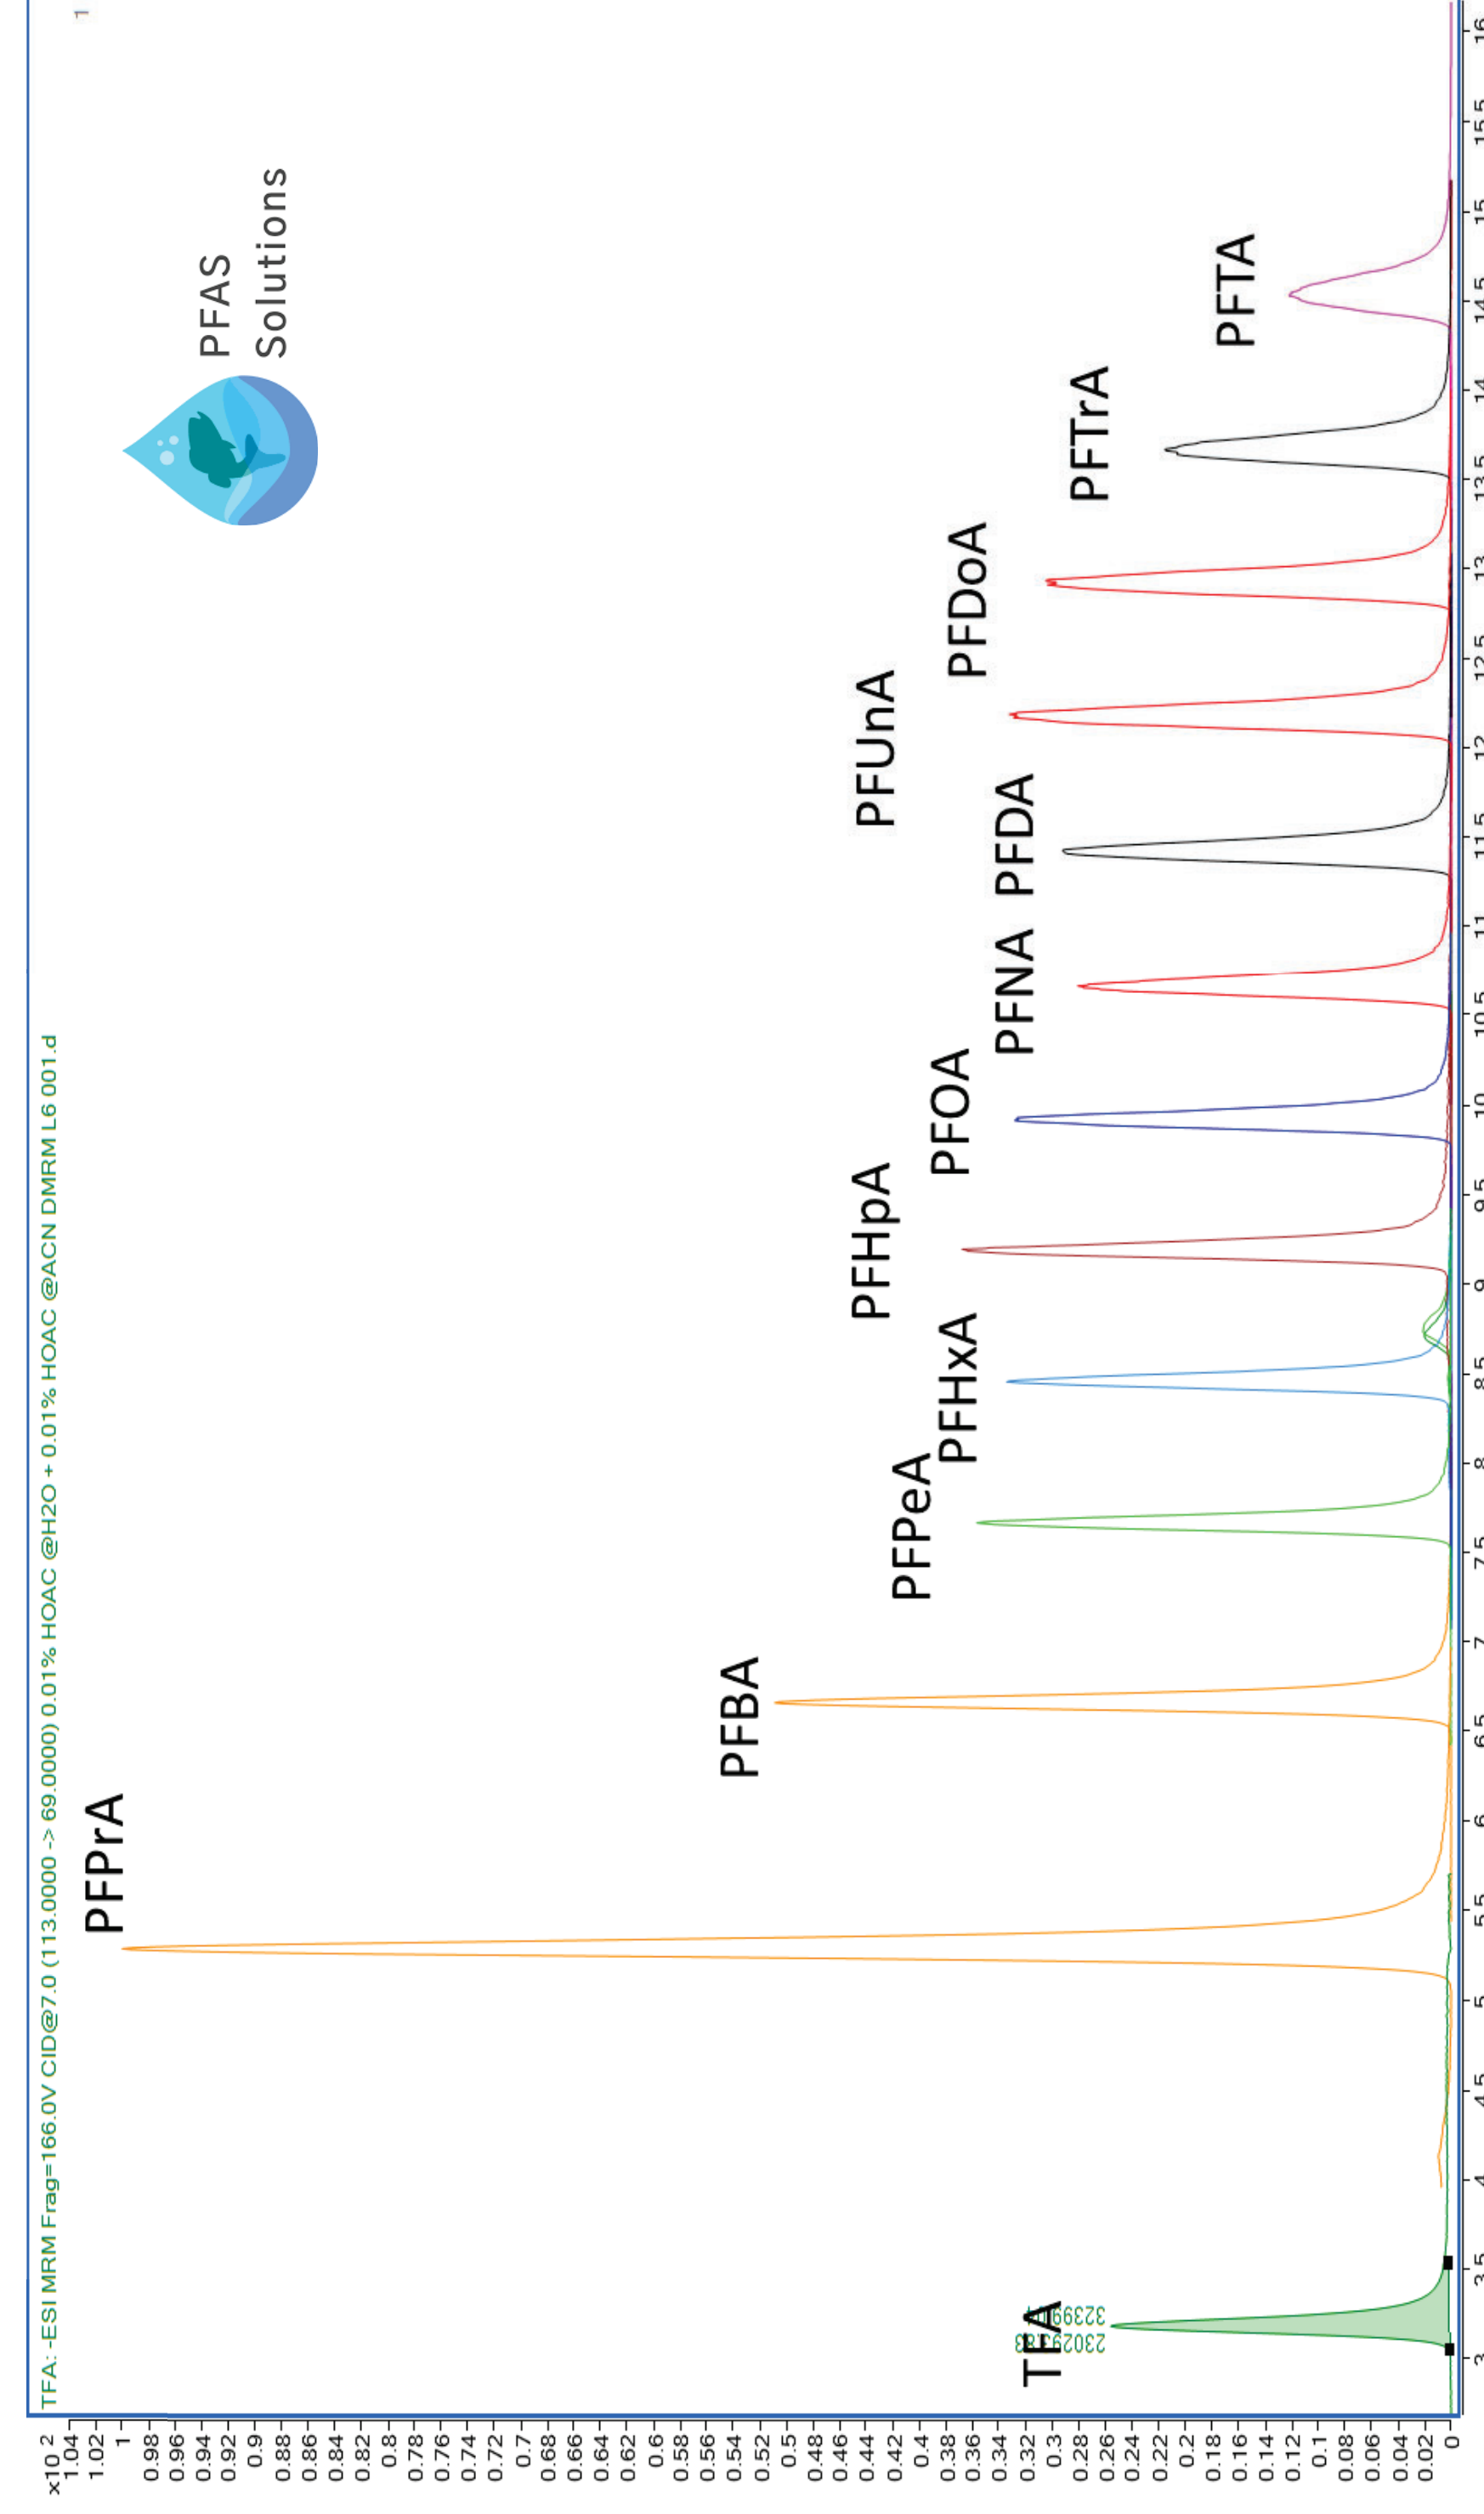

A separation of short chain PFAS is performed using acetic acid as an acidic modifier. Adequate retention and peak shape is observed while maintaining resolution for other long chain PFAS compounds.

Parameter	Value
Flow Rate	0.5 mL/min
Oven Temperature	40°C
Injection volume	2 µL
MPA	0.01% HOAc in water
MPB	0.01% HOAc in ACN

Time (min)	% MPA	% MPB
0	80	20
5	20	80
12	10	90
18	10	90
18.1	80	20

Conclusions

A new positive charge surface (PCS) stationary phase from Advanced Materials Technology shows adequate retention and peak shape for short chain PFAS analytes such as TFA and PFPPA in combination with a HALO PFAS Delay column.

The superficially porous particle technology shows an advantage in peak widths due to the solid silica core when compared to fully porous particle material.

Future work will include LOD experiments along with temperature comparisons in order to speed up the analysis time. Moving the column dimension down to a 1.5mm ID will also be explored in order to boost sensitivity while reducing solvent consumption.

HALO® is a registered trademark of Advanced Materials Technology, Inc